



PGD Micro Capsule Filters

Pleated Fiberglass Depth Media

PGD Micro Capsule filters are constructed with fiberglass depth media for clarification and prefiltration of aqueous liquids. Pore sizes range from 0.22 to 5.0 μm . Additional filter devices scale from laboratory to full production using identical materials to ensure consistent results.

Designed to meet FDA requirements, PGD Micro Capsules are manufactured to ensure fiber free effluent. They are rated at 99% retention at the indicated pore size. PGD Micro Capsule filters offer the benefits of high flow rates, high contaminant holding capacity as well as excellent retention. These hydrophilic, high capacity filters are used in pre-filter applications as well as final filter applications where the goal is bioburden reduction and not sterile product. PGD Micro Capsules are available pre-sterilized.

Critical Process provides unrivaled delivery times, technical consulting before purchasing, and very competitively priced high-performance products. Our comprehensive testing & analysis and validation services support your team whenever they need it. Your process experts partnering with our filtration experts is how we deliver your company's solution right the first time.

Clarification & Prefiltration

Particle Filtration




MICRO CAPSULES – Nominal Dimensions

Body Length: 1.9 in. (4.8 cm)

Overall Length: 2.8 to 3.8 in. (7.1 to 9.7 cm)

Outside Diameter: 2.6 in. (6.6 cm)

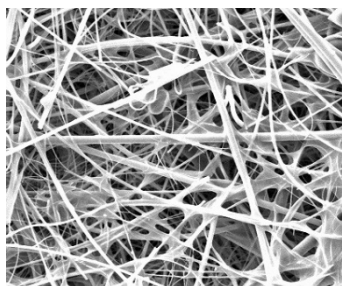

PGD Micro Capsules are recommended for clarification & prefiltration in:

- Intermediates
- Buffers & Growth Media
- Bulk Pharmaceutical Chemicals
- LVPs & SVPs
- WFI, Water Purification

Maximum Operating Parameters

	MICRO CAPSULES
Liquid Operational Pressure	80 psi at 68 °F (5.52 bard at 20 °C)
Gases Operational Pressure	60 psi at 68 °F (4.14 bar at 20 °C)
Operating Temperature (water)	110 °F at 30 psid (43 °C at 2.07 bard)
Forward Differential Pressure	50 psid at 68 °F (3.45 bard at 20 °C)
Reverse Differential Pressure	40 psid at 68 °F (2.76 bard at 20 °C)
Recommended Changeout Pressure	35 psid (2.41 bard)

Sanitization & Sterilization

Autoclave	250 °F (121 °C), 30 min, 5+ cycles
Chemical Sanitization	Performed using industry standard concentrations of hydrogen peroxide, peracetic acid, sodium hypochlorite and other selected chemicals.

Filtration Area (Nominal)

	Pleated Depth Media
Area	0.476 ft ²
	442 cm ²

Construction Materials

Filtration Media	Pleated Fiberglass Depth Media
Media Support	Polyester
End Caps, Center Core, Outer Support Cage, Micro Capsule Housing	Polypropylene
Sealing Method	Thermal Bonding

Endotoxins

The levels of bacterial endotoxins in aqueous extracts from PGD Micro Capsule filters are below current USP limits as specified for water for injection.

Extractables

PGD Micro Capsule filters typically exhibit low levels of non-volatile residues.

TOC and Conductivity

PGD Micro Capsule filters conform with TOC standards of USP <643> and the water conductivity standards of USP <645> after an appropriate flush with purified water.

Toxicity Compliance

Materials used to construct PGD Micro Capsule filters are non-toxic and meet the requirements for the MEM Elution Cytotoxicity Test and the requirements for Biological Reactivity Tests in the current version of the United States Pharmacopeia (USP) for Class VI - 121 °C Plastics.


Non-Fiber Releasing

PGD Micro Capsule filters comply with Title 21 CFR sections 210.3 (b)(6) and 211.72, for non-fiber releasing filters.

FDA Compliance

Materials meet the requirements listed by the FDA as appropriate for use in articles intended for repeated food contact as specified in Title 21 CFR sections 174.5, 177.1500, 177.1520, 177.1630, 177.2440, and 177.2600 as applicable.

Flow Rates for PGD Micro Capsules by Pore Size

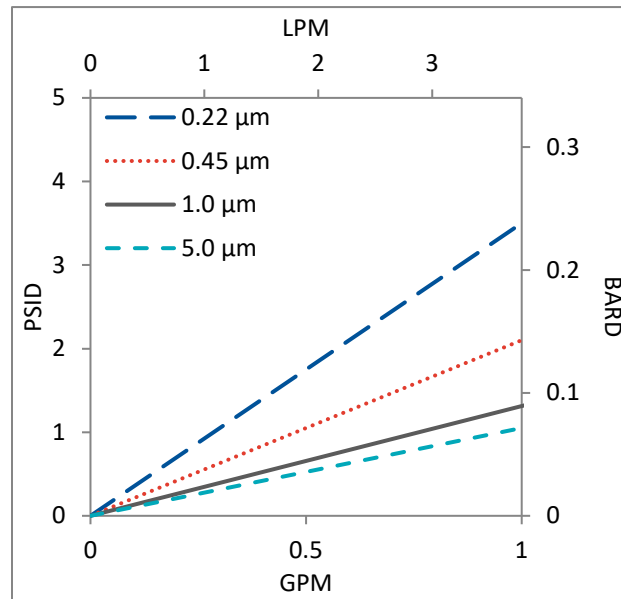

Flow rates for Micro Capsule filters are per filter. The test fluid is water at ambient temperature. Flows are tested using a Micro capsule filter with ½" Sanitary inlet and outlet ports. Rates will vary based on end configuration of the Micro capsule.

PGD Micro Capsule Filters Ordering Information

All Critical Process filters are configurable to meet customer specifications. Fill in the corresponding codes in the boxes below to build your Part Number.

To consult with one of our technical team members, request a quote or place an order: call (603) 880-4420 or [contact us here](#).

Micro Capsule Filters

MIC PGD 000 -

Pore Size Code -20 = 0.22 µm -40 = 0.45 µm 1-0 = 1.0 µm 5-0 = 5.0 µm	Pre-Sterilized or Not S = Pre-Sterilized N = Not Sterilized	Inlet 1 = 1/8" Hose Barb 2 = 1/4" Hose Barb 3 = 1/2" Hose Barb 4 = Luer Lock 5 = 1/2" Sanitary* 6 = 1/4" MNPT	Inlet Vent Port 1 = 1/8" Hose Barb 2 = 1/4" Hose Barb 3 = 1/2" Hose Barb 4 = Luer Lock 6 = 1/4" MNPT 7 = Side Bleed Valve	Outlet 1 = 1/8" Hose Barb 2 = 1/4" Hose Barb 3 = 1/2" Hose Barb 3B = 1/2" Hose Barb with Filling Bell 4 = Luer Lock 5 = 1/2" Sanitary* 6 = 1/4" MNPT	Outlet Vent Port 1 = 1/8" Hose Barb 2 = 1/4" Hose Barb 3 = 1/2" Hose Barb 4 = Luer Lock 6 = 1/4" MNPT 7 = Side Bleed Valve	Side Vent O-Ring** B = Buna E = EP S = Silicone V = Viton (or FKM) K = FFKM
---	--	--	--	--	---	---

*When choosing the Sanitary Inlet/Outlet, the Luer Lock or bleed valve option is required for the Vent Port
 ** O-Ring is only available on Bleed Valve



One Chestnut Street
 Nashua, NH 03060
 603.880.4420
 FAX: 603.880.4536

CriticalProcess.com

The information contained herein is subject to change without notice. The Critical Process Filtration logo is a trademark of Critical Process Filtration, Inc. Viton is a trademark of DuPont Performance Elastomers L.L.C.
 © 2025 Critical Process Filtration, Inc. • All Rights Reserved

Data Sheet PGD Micro DS Rev -